

Алматы (7273)495-231
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70


Казахстан +7(7172)727-132

Киргизия +996(312)96-26-47

<https://biochromato.nt-rt.ru> || boa@nt-rt.ru



Thermal Desorption and Pyrolysis for DART®-MS

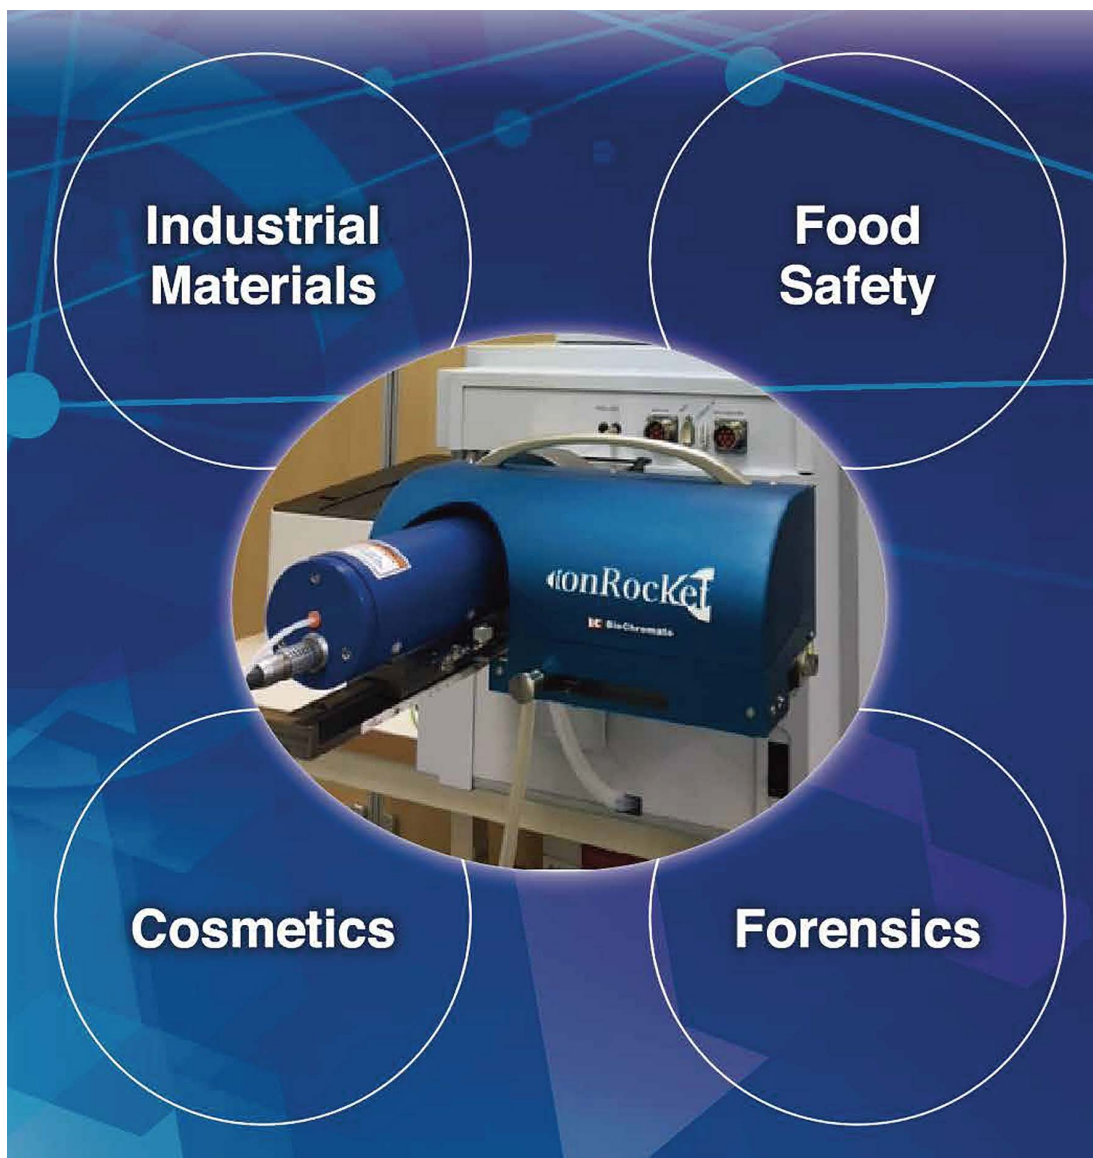




8Connect to DART®-MS and Visualize Hidden Compounds

8Temperature Gradient System Visualizes Compounds in Real Time

- Eliminates Sample Preparation Steps

8Great for Polymer Analysis

ionRocket DART® -MS System

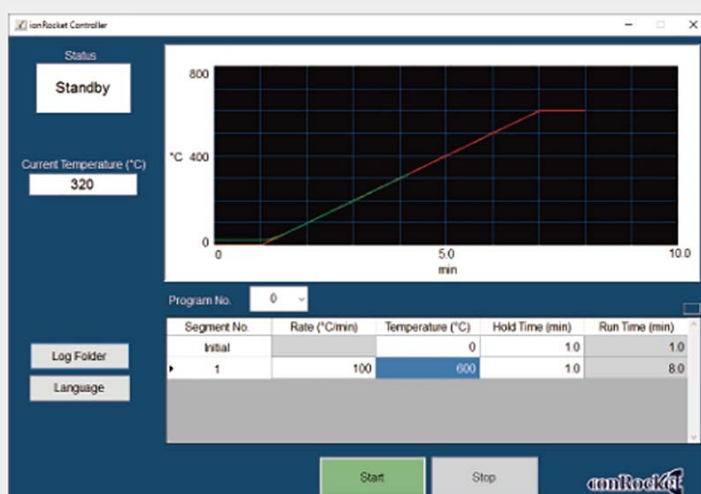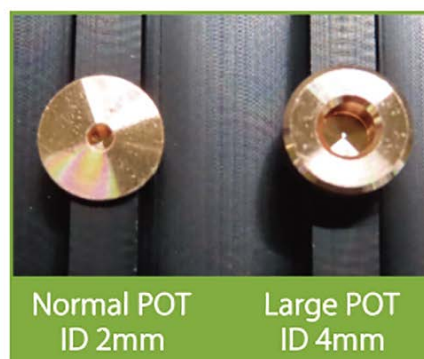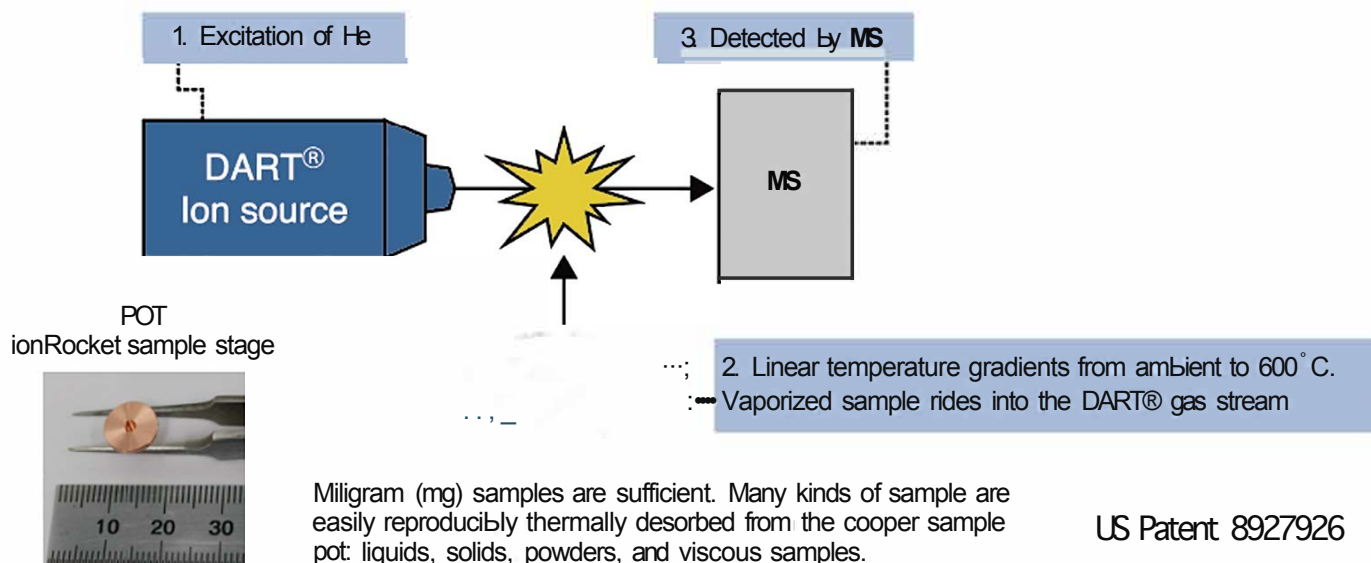

ionRocket generates a temperature gradient from ambient up to as high as 600° C over several minutes.

This allows compounds in your samples to be sublimated, vaporized, or pyrolyzed according to their volatility, and then introduced into the DART® gas stream.

Analysis of polyethylene terephthalate (PET)

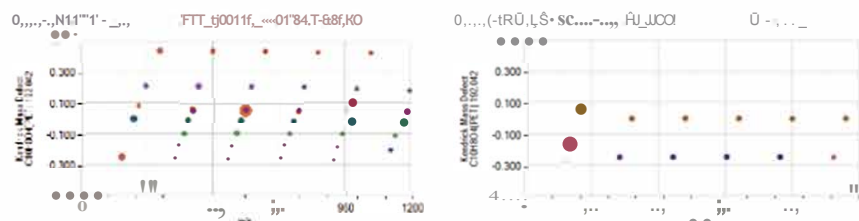


Fig.1 Bubble plots (500 °C) of repeating unit in PET A and B

Purpose

Analysis of polyethylene terephthalate (PET) used in PET bottles using a time-of-flight mass spectrometer as a detector

Experiment

MS measurement of small pieces of PET bottles (A, B) using the ionRocket while raising the temperature from room temperature to 500 °C (A; hard PET B; soft PET)

Analysis method

Using Spectra Scope and Data Analysis software, PET repeating structures were extracted from mass spectra, and A and B PET were compared.

Results

Fig.1 shows the analysis results (bubble plot) of the Polymer engine. It was found that A had more PET repeating structures ($C_{10}H_8O_4$) than B.

Figure 2 shows the TIC and mass spectra. B was found to be more thermally decomposed than A. These results seem to indicate differences in the degree of polymerization and hardness of PET. It could be detected without pretreatment that the difference in the degree of polymerization and the characteristics of PET from PET bottles insoluble in general solvents.

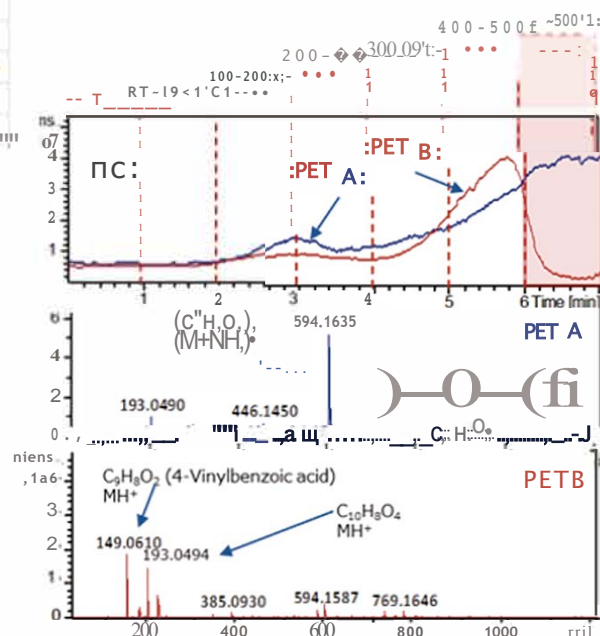


Fig.2 TIC and mass spectra of PET A and B (500 °C)

Comparison analysis of laser printer prints

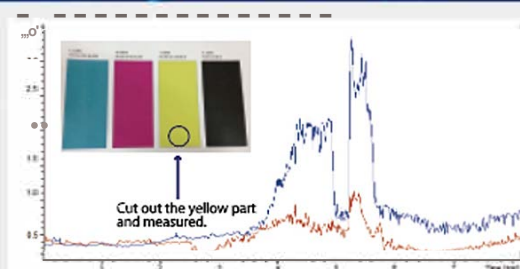


Fig.1 TIC of printed yellow part on paper

RT	m/z	Intensity	Reference	Sample Area	Score	Compound Result
4.01-4.99	123.068	93422	81016	39522	922	3
4.01-4.99	111.049	60891	71999	94601	194	3
5.01-5.99	175.1114	100192	1616	542622	975	2
4.01-4.99	115.0797	80899	23166	216252	89.1	2
5.01-5.99	109.0283	288519	228262	1290588	82.6	2
3.01-3.99	355.2841	151822	4430	529826	99.2	1
4.01-4.99	265.0633	50344	2448	138170	98.2	1
4.01-4.99	387.1271	248400	582	2596232	100	1
5.01-5.99	163.0387	76784	99691	353155	111	1

Fig.2 IDS Result Table

Purpose

Using a time-of-flight mass spectrometer as a detector, comparative analysis was performed between the two models with the yellow part printed by a laser printer.

Experiment

A yellow color code was printed, cut out to a diameter of 3 mm, and two pieces were measured with ionRocket while raising the temperature from room temperature to 600 °C.

Analysis method

The differences between samples were examined using "IDS" * (Intelligent Data Subtraction) of "Spectra Scope". The composition of peaks with differences was analyzed, and the compounds were estimated by "Compound Search".

Results

Fig.1 shows the TIC of Sample A (red) and B (blue). When the difference analysis was performed using "IDS" of "Spectra Scope", differences were found in multiple compounds (Figs. 2, 3). Among the difference components, $m/z=387.1271$ was detected in the printed paper Sample B around 4 to 5 minutes (300 to 400 °C), and $C_{18}H_{18}N_4O_6$ seemed to be the most consistent by composition analysis. The compound was estimated as "Pigment Yellow 74" by "Compound Search". With ionRocket, printed materials can be directly measured without sample preparation, making it easy to perform difference analysis and compound estimation.

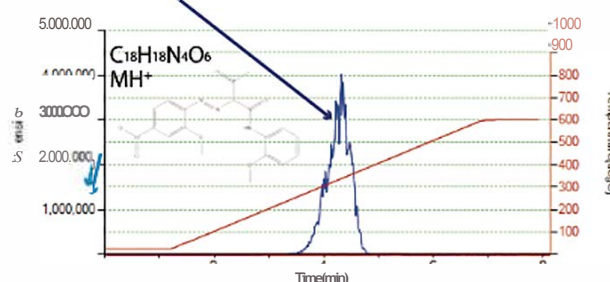


Fig.3 EIC of $m/z=387.1271$

Specifications

Main body



Heater control box



Heater control software



POT (50pc) included



Product name	ionRocket
Catalog Code	MSIR04
Main Body outer dimension/weight	W: 315 mm x D: 120 mm x H: 175 mm / 3.2 kg
Heater control box dimension/weight	W: 321 mm x D: 220 mm x H: 147 mm / 4.1 kg
Heating control temperature	Room temperature to 600 °C
Main power	AC100V-240V, 50Hz/60 Hz
Operating temperature environment	10 °C to 40 °C (No condensation)
Power consumption	During operation: 320 W As stand-by: 32 W

* Note that the content and/or specifications described in this catalog may be subject to change without notice.

Алматы (7273)495-231
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922)49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Иваново (4932)77-34-06
Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Саранск (8342)22-96-24
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сургут (3462)77-98-35
Сыктывкар (8212)25-95-17
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Тольятти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Улан-Удэ (3012)59-97-51
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чеховсары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93

Россия +7(495)268-04-70

Казахстан +7(7172)727-132

Киргизия +996(312)96-26-47

<https://biochromato.nt-rt.ru> || boa@nt-rt.ru